

# AQ-SPEC

## Air Quality Sensor Performance Evaluation Center

### Sensor Description

Manufacturer/Model:  
Aeroqual S-500 OZU

Pollutant: Ozone

Measurement Range:  
0-0.15 ppm

Type: Metal Oxide

Time Resolution: 1 Minute



### Additional Information

Field evaluation report:  
<http://www.aqmd.gov/aq-spec/evaluations/field>

Lab evaluation report:  
<http://www.aqmd.gov/aq-spec/evaluations/laboratory>



AQ-SPEC website:  
<http://www.aqmd.gov/aq-spec>

### Evaluation Summary

- Overall, the three Aeroqual sensors showed high accuracy, compared to the FRM ozone monitor, for a concentration range between 0 to 150 ppb.
- The three Aeroqual sensors exhibited high precision during most of the tested environmental conditions. Except for high temperature and humidity, sensors had some difficulties recording low concentration ozone.
- The three Aeroqual sensors showed low intra-model variability, as well as good data recovery (100%).
- They showed strong correlations with the FRM instrument from the field ( $R^2 > 0.85$ ) and very strong correlations from the laboratory studies ( $R^2 > 0.99$ ).

### Field Evaluation Highlights

- Deployment period 02/10/2015- 04/04/2015: the three Aeroqual sensors followed the ozone concentration change as monitored by FRM instrument.
- The units showed 100% data recovery.
- The units have low intra-model variability (+/- 10%).

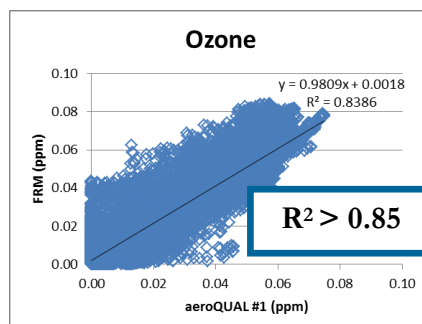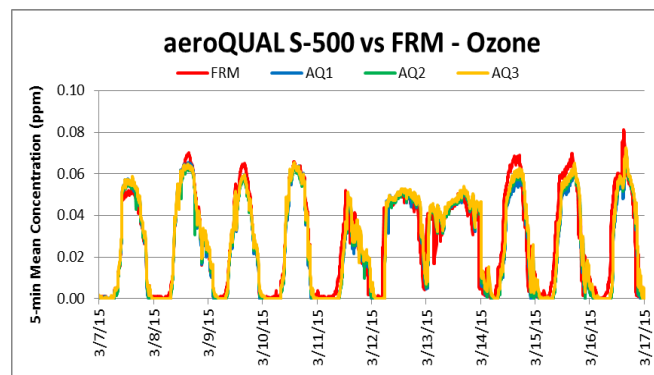

Coefficient of determination ( $R^2$ ) quantifies how the three sensors followed the ozone concentration change by FRM.

An  $R^2$  approaching the value of 1 reflects a near perfect agreement, whereas a value of 0 indicates a complete lack of correlation.

# Laboratory Evaluation Highlights

## Accuracy

$$A (\%) = 100 - \frac{|\bar{X} - \bar{R}|}{\bar{R}} * 100$$


Steady State (#)	Sensor mean (ppb)	FRM (ppb)	Accuracy (%)
1	31.7	28.0	86.8
2	53.6	57.6	93.1
3	73.4	88.4	83.0

Accuracy was evaluated by a concentration ramping experiment at 20 °C and 40%. The sensor's readings at each ramping steady state are compared to the reference instrument.

Negative % means sensors' overestimation by more than two fold. The higher the positive value (close to 100%), the higher the sensor's accuracy.




## Precision

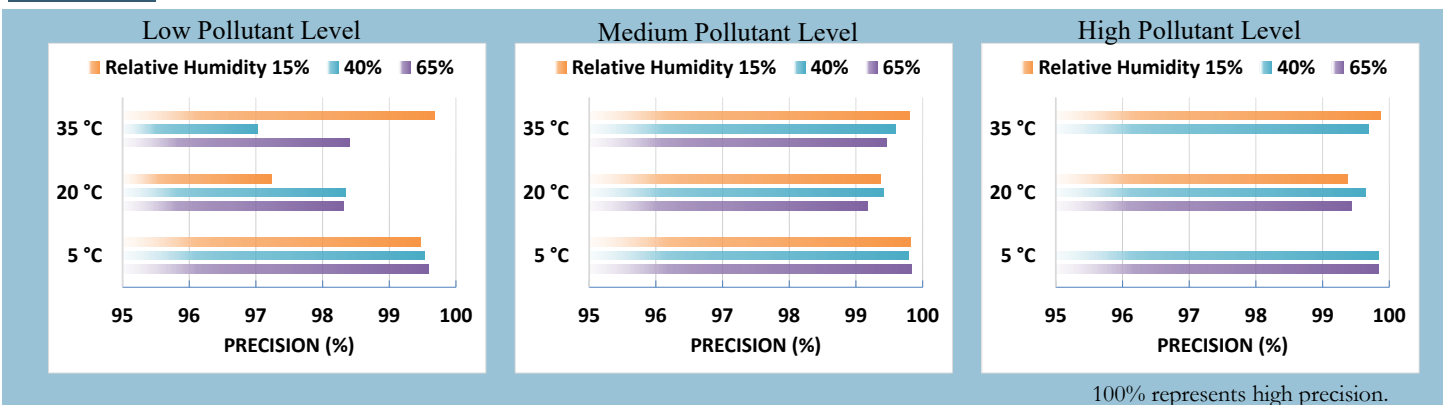

Sensor's ability of generating precise measurements of ozone concentration at low, medium, and high pollutant levels were evaluated under 9 combinations of T and RH, including extreme weather conditions like cold and humid (5 °C and 65%), hot and humid (35 °C and 65%), or hot and dry (35 °C and 15%).

## Coefficient of Determination

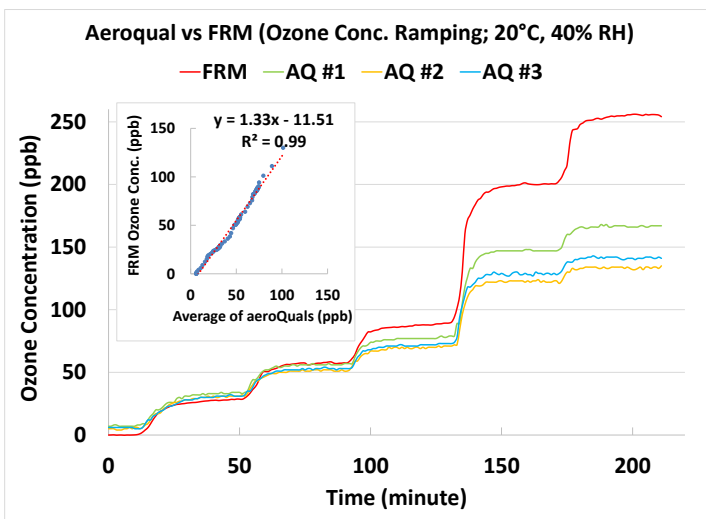

The three Aeroqual sensors showed very strong correlations with the corresponding FRM data ( $R^2 > 0.99$ ) at 20 °C and 40% RH

## Climate Susceptibility ( $R^2$ )

$R^2$	5 °C	20 °C	35 °C
15%	0.97	0.98	0.99
40%	0.95	0.99	0.99
65%	0.99	0.98	0.96

## Observed Interferents

High temperature coupled with high humidity.



All documents, reports, data, and other information provided in this document are for informational use only. Mention of trade names or commercial products does not constitute endorsement or recommendation. The South Coast AQMD's AQ-SPEC program, as a government agency, recommends the interested parties to make purchase decisions based on their application.